

In-situ calibration of the single-photoelectron charge response of the IceCube photomultiplier tubes



IceCube collaboration

M. G. Aartsen,^p M. Ackermann,^{bc} J. Adams,^p J. A. Aguilar,^l M. Ahlers,^t M. Ahrens,^{at}
C. Alispach,^z K. Andeen,^{ak} T. Anderson,^{az} I. Ansseau,^l G. Anton,^x C. Argüelles,ⁿ
J. Auffenberg,^a S. Axani,ⁿ P. Backes,^a H. Bagherpour,^p X. Bai,^{aq} A. Balagopal V.,^{ac}
A. Barbano,^z S. W. Barwick,^{ab} B. Bastian,^{bc} V. Baum,^{aj} S. Baur,^l R. Bay,^h J. J. Beatty,^{r,s}
K.-H. Becker,^{bb} J. Becker Tjus,^k S. BenZvi,^{as} D. Berley,^q E. Bernardini,^{bc,bd}
D. Z. Besson,^{ad,be} G. Binder,^{h,i} D. Bindig,^{bb} E. Blaufuss,^q S. Blot,^{bc} C. Boehm,^{at} M. Börner,^u
S. Böser,^{aj} O. Botner,^{ba} J. Böttcher,^a E. Bourbeau,^t J. Bourbeau,^{ai} F. Bradascio,^{bc}
J. Braun,^{ai} S. Bron,^z J. Brostean-Kaiser,^{bc} A. Burgman,^{ba} J. Buscher,^a R. S. Busse,^{al}
T. Carver,^z C. Chen,^f E. Cheung,^q D. Chirkin,^{ai} S. Choi,^{av} K. Clark,^{ae} L. Classen,^{al}
A. Coleman,^{am} G. H. Collin,ⁿ J. M. Conrad,ⁿ P. Coppin,^m P. Correa,^m D. F. Cowen,^{ay,az}
R. Cross,^{as} P. Dave,^f C. De Clercq,^m J. J. DeLaunay,^{az} H. Dembinski,^{am} K. Deoskar,^{at}
S. De Ridder,^{aa} P. Desiati,^{ai} K. D. de Vries,^m G. de Wasseige,^m M. de With,^j T. DeYoung,^v
A. Diaz,ⁿ J. C. Díaz-Vélez,^{ai} H. Dujmovic,^{av} M. Dunkman,^{az} E. Dvorak,^{aq} B. Eberhardt,^{ai}
T. Ehrhardt,^{aj} P. Eller,^{az} R. Engel,^{ac} P. A. Evenson,^{am} S. Fahey,^{ai} A. R. Fazely,^g J. Felde,^q
K. Filimonov,^h C. Finley,^{at} D. Fox,^{ay} A. Franckowiak,^{bc} E. Friedman,^q A. Fritz,^{aj}
T. K. Gaisser,^{am} J. Gallagher,^{ah} E. Ganster,^a S. Garrappa,^{bc} L. Gerhardt,ⁱ K. Ghorbani,^{ai}
T. Glauch,^y T. Glüsenkamp,^x A. Goldschmidt,ⁱ J. G. Gonzalez,^{am} D. Grant,^v Z. Griffith,^{ai}
S. Griswold,^{as} M. Gündler,^a M. Gündüz,^k C. Haack,^a A. Hallgren,^{ba} L. Halve,^a F. Halzen,^{ai}
K. Hanson,^{ai} A. Haungs,^{ac} D. Hebecker,^j D. Heereman,^l P. Heix,^a K. Helbing,^{bb} R. Hellauer,^q
F. Henningsen,^y S. Hickford,^{bb} J. Hignight,^w G. C. Hill,^b K. D. Hoffman,^q R. Hoffmann,^{bb}
T. Hoinka,^u B. Hokanson-Fasig,^{ai} K. Hoshina,^{ai,be} F. Huang,^{az} M. Huber,^y T. Huber,^{ac,bc}
K. Hultqvist,^{at} M. Hünnefeld,^u R. Hussain,^{ai} S. In,^{av} N. Iovine,^l A. Ishihara,^o
G. S. Japaridze,^e M. Jeong,^{av} K. Jero,^{ai} B. J. P. Jones,^d F. Jonske,^a R. Joppe,^a D. Kang,^{ac}
W. Kang,^{av} A. Kappes,^{al} D. Kappesser,^{aj} T. Karg,^{bc} M. Karl,^y A. Karle,^{ai} U. Katz,^x
M. Kauer,^{ai} J. L. Kelley,^{ai} A. Kheirandish,^{ai} J. Kim,^{av} T. Kintscher,^{bc} J. Kiryluk,^{au} T. Kittler,^x
S. R. Klein,^{h,i} R. Koirala,^{am} H. Kolanoski,^j L. Köpke,^{aj} C. Kopper,^v S. Kopper,^{ax}
D. J. Koskinen,^t M. Kowalski,^{j,bc} K. Krings,^y G. Krückl,^{aj} N. Kulacz,^w N. Kurahashi,^{ap}
A. Kyriacou,^b M. Labare,^{aa} J. L. Lanfranchi,^{az} M. J. Larson,^q F. Lauber,^{bb} J. P. Lazar,^{ai}
K. Leonard,^{ai} A. Leszczyńska,^{ac} M. Leuermann,^a Q. R. Liu,^{ai} E. Lohfink,^{aj}

C. J. Lozano Mariscal,^{al} L. Lu,^o F. Lucarelli,^z J. Lünemann,^m W. Luszczak,^{ai} Y. Lyu,^{h,i} W. Y. Ma,^{bc} J. Madsen,^{ar} G. Maggi,^m K. B. M. Mahn,^v Y. Makino,^o P. Mallik,^a K. Mallot,^{ai} S. Mancina,^{ai} I. C. Mariş,^l R. Maruyama,^{an} K. Mase,^o R. Maunu,^q F. McNally,^{ag} K. Meagher,^{ai} M. Medici,^t A. Medina,^s M. Meier,^u S. Meighen-Berger,^y T. Menne,^u G. Merino,^{ai} T. Meures,^l J. Micallef,^v D. Mockler,^l G. Momenté,^{aj} T. Montaruli,^z R. W. Moore,^w R. Morse,^{ai} M. Moulai,ⁿ P. Muth,^a R. Nagai,^o U. Naumann,^{bb} G. Neer,^v H. Niederhausen,^y M. U. Nisa,^v S. C. Nowicki,^v D. R. Nygren,ⁱ A. Obertacke Pollmann,^{bb} M. Oehler,^{ac} A. Olivas,^q A. O’Murchadha,^l E. O’Sullivan,^{at} T. Palczewski,^{h,i} H. Pandya,^{am} D. V. Pankova,^{az} N. Park,^{ai} P. Peiffer,^{aj} C. Pérez de los Heros,^{ba} S. Philippen,^a D. Pieloth,^u E. Pinat,^l A. Pizzuto,^{ai} M. Plum,^{ak} A. Porcelli,^{aa} P. B. Price,^h G. T. Przybylski,ⁱ C. Raab,^l A. Raissi,^p M. Rameez,^t L. Rauch,^{bc} K. Rawlins,^c I. C. Rea,^y R. Reimann,^a B. Relethford,^{ap} M. Renschler,^{ac} G. Renzi,^l E. Resconi,^y W. Rhode,^u M. Richman,^{ap} S. Robertson,ⁱ M. Rongen,^a C. Rott,^{av} T. Ruhe,^u D. Ryckbosch,^{aa} D. Rysewyk,^v I. Safa,^{ai} S. E. Sanchez Herrera,^v A. Sandrock,^u J. Sandros,^{aj} M. Santander,^{ax} S. Sarkar,^{ao} S. Sarkar,^w K. Satalecka,^{bc} M. Schaufel,^a H. Schieler,^{ac} P. Schlunder,^u T. Schmidt,^q A. Schneider,^{ai} J. Schneider,^x F. G. Schröder,^{ac,am} L. Schumacher,^a S. Sclafani,^{ap} D. Seckel,^{am} S. Seunarine,^{ar} S. Shefali,^a M. Silva,^{ai} R. Snihur,^{ai} J. Soedingrekso,^u D. Soldin,^{am} M. Song,^q G. M. Spiczak,^{ar} C. Spiering,^{bc} J. Stachurska,^{bc} M. Stamatikos,^s T. Stanev,^{am} R. Stein,^{bc} P. Steinmüller,^{ac} J. Stettner,^a A. Steuer,^{aj} T. Stezelberger,ⁱ R. G. Stokstad,ⁱ A. Stöbl,^o N. L. Strotjohann,^{bc} T. Stürwald,^a T. Stuttard,^t G. W. Sullivan,^q I. Taboada,^f F. Tenholt,^k S. Ter-Antonyan,^g A. Terliuk,^{bc} S. Tilav,^{am} K. Tollefson,^v L. Tomankova,^k C. Tönnis,^{aw} S. Toscano,^l D. Tosi,^{ai} A. Trettin,^{bc} M. Tselengidou,^x C. F. Tung,^f A. Turcati,^y R. Turcotte,^{ac} C. F. Turley,^{az} B. Ty,^{ai} E. Unger,^{ba} M. A. Unland Elorrieta,^{al} M. Usner,^{bc} J. Vandenbroucke,^{ai} W. Van Driessche,^{aa} D. van Eijk,^{ai} N. van Eijndhoven,^m S. Vanheule,^{aa} J. van Santen,^{bc} M. Vraeghe,^{aa} C. Walck,^{at} A. Wallace,^b M. Wallraff,^a N. Wandkowsky,^{ai} T. B. Watson,^d C. Weaver,^w A. Weindl,^{ac} M. J. Weiss,^{az} J. Weldert,^{aj} C. Wendt,^{ai} J. Werthebach,^{ai} B. J. Whelan,^b N. Whitehorn,^{af} K. Wiebe,^{aj} C. H. Wiebusch,^a L. Wille,^{ai} D. R. Williams,^{ax} L. Wills,^{ap} M. Wolf,^y J. Wood,^{ai} T. R. Wood,^w K. Woschnagg,^h G. Wrede,^x D. L. Xu,^{ai} X. W. Xu,^g Y. Xu,^{au} J. P. Yanez,^w G. Yodh,^{ab} S. Yoshida,^o T. Yuan^{ai} and M. Zöcklein^a

^a*III. Physikalisches Institut, RWTH Aachen University, D-52056 Aachen, Germany*

^b*Department of Physics, University of Adelaide, Adelaide, 5005, Australia*

^c*Dept. of Physics and Astronomy, University of Alaska Anchorage, 3211 Providence Dr., Anchorage, AK 99508, USA*

^d*Dept. of Physics, University of Texas at Arlington, 502 Yates St., Science Hall Rm 108, Box 19059, Arlington, TX 76019, USA*

^e*CTSPS, Clark-Atlanta University, Atlanta, GA 30314, USA*

^f*School of Physics and Center for Relativistic Astrophysics, Georgia Institute of Technology, Atlanta, GA 30332, USA*

^g*Dept. of Physics, Southern University, Baton Rouge, LA 70813, USA*

^h*Dept. of Physics, University of California, Berkeley, CA 94720, USA*

ⁱ*Lawrence Berkeley National Laboratory, Berkeley, CA 94720, USA*

^j*Institut für Physik, Humboldt-Universität zu Berlin, D-12489 Berlin, Germany*

^k*Fakultät für Physik & Astronomie, Ruhr-Universität Bochum, D-44780 Bochum, Germany*

¹ *Université Libre de Bruxelles, Science Faculty CP230, B-1050 Brussels, Belgium*

^m *Vrije Universiteit Brussel (VUB), Dienst ELEM, B-1050 Brussels, Belgium*

ⁿ *Dept. of Physics, Massachusetts Institute of Technology, Cambridge, MA 02139, USA*

^o *Dept. of Physics and Institute for Global Prominent Research, Chiba University, Chiba 263-8522, Japan*

^p *Dept. of Physics and Astronomy, University of Canterbury, Private Bag 4800, Christchurch, New Zealand*

^q *Dept. of Physics, University of Maryland, College Park, MD 20742, USA*

^r *Dept. of Astronomy, Ohio State University, Columbus, OH 43210, USA*

^s *Dept. of Physics and Center for Cosmology and Astro-Particle Physics, Ohio State University, Columbus, OH 43210, USA*

^t *Niels Bohr Institute, University of Copenhagen, DK-2100 Copenhagen, Denmark*

^u *Dept. of Physics, TU Dortmund University, D-44221 Dortmund, Germany*

^v *Dept. of Physics and Astronomy, Michigan State University, East Lansing, MI 48824, USA*

^w *Dept. of Physics, University of Alberta, Edmonton, Alberta, Canada T6G 2E1*

^x *Erlangen Centre for Astroparticle Physics, Friedrich-Alexander-Universität Erlangen-Nürnberg, D-91058 Erlangen, Germany*

^y *Physik-department, Technische Universität München, D-85748 Garching, Germany*

^z *Département de physique nucléaire et corpusculaire, Université de Genève, CH-1211 Genève, Switzerland*

^{aa} *Dept. of Physics and Astronomy, University of Gent, B-9000 Gent, Belgium*

^{ab} *Dept. of Physics and Astronomy, University of California, Irvine, CA 92697, USA*

^{ac} *Karlsruhe Institute of Technology, Institut für Kernphysik, D-76021 Karlsruhe, Germany*

^{ad} *Dept. of Physics and Astronomy, University of Kansas, Lawrence, KS 66045, USA*

^{ae} *SNOLAB, 1039 Regional Road 24, Creighton Mine 9, Lively, ON, Canada P3Y 1N2*

^{af} *Department of Physics and Astronomy, UCLA, Los Angeles, CA 90095, USA*

^{ag} *Department of Physics, Mercer University, Macon, GA 31207-0001, USA*

^{ah} *Dept. of Astronomy, University of Wisconsin, Madison, WI 53706, USA*

^{ai} *Dept. of Physics and Wisconsin IceCube Particle Astrophysics Center, University of Wisconsin, Madison, WI 53706, USA*

^{aj} *Institute of Physics, University of Mainz, Staudinger Weg 7, D-55099 Mainz, Germany*

^{ak} *Department of Physics, Marquette University, Milwaukee, WI, 53201, USA*

^{al} *Institut für Kernphysik, Westfälische Wilhelms-Universität Münster, D-48149 Münster, Germany*

^{am} *Bartol Research Institute and Dept. of Physics and Astronomy, University of Delaware, Newark, DE 19716, USA*

^{an} *Dept. of Physics, Yale University, New Haven, CT 06520, USA*

^{ao} *Dept. of Physics, University of Oxford, Parks Road, Oxford OX1 3PU, UK*

^{ap} *Dept. of Physics, Drexel University, 3141 Chestnut Street, Philadelphia, PA 19104, USA*

^{aq} *Physics Department, South Dakota School of Mines and Technology, Rapid City, SD 57701, USA*

^{ar} *Dept. of Physics, University of Wisconsin, River Falls, WI 54022, USA*

^{as} *Dept. of Physics and Astronomy, University of Rochester, Rochester, NY 14627, USA*

^{at} *Oskar Klein Centre and Dept. of Physics, Stockholm University, SE-10691 Stockholm, Sweden*

^{au} *Dept. of Physics and Astronomy, Stony Brook University, Stony Brook, NY 11794-3800, USA*

^{av} *Dept. of Physics, Sungkyunkwan University, Suwon 16419, Korea*

^{aw} *Institute of Basic Science, Sungkyunkwan University, Suwon 16419, Korea*

^{ax} *Dept. of Physics and Astronomy, University of Alabama, Tuscaloosa, AL 35487, USA*

^{ay} *Dept. of Astronomy and Astrophysics, Pennsylvania State University, University Park, PA 16802, USA*

^{az}*Dept. of Physics, Pennsylvania State University, University Park, PA 16802, USA*

^{ba}*Dept. of Physics and Astronomy, Uppsala University, Box 516, S-75120 Uppsala, Sweden*

^{bb}*Dept. of Physics, University of Wuppertal, D-42119 Wuppertal, Germany*

^{bc}*DESY, D-15738 Zeuthen, Germany*

^{bd}*also at Università di Padova, I-35131 Padova, Italy*

^{be}*also at National Research Nuclear University, Moscow Engineering Physics Institute (MEPhI), Moscow 115409, Russia*

^{bf}*Earthquake Research Institute, University of Tokyo, Bunkyo, Tokyo 113-0032, Japan*

E-mail: analysis@icecube.wisc.edu

ABSTRACT: We describe an improved in-situ calibration of the single-photoelectron charge distributions for each of the in-ice Hamamatsu Photonics R7081-02[MOD] photomultiplier tubes in the IceCube Neutrino Observatory. The characterization of the individual PMT charge distributions is important for PMT calibration, data and Monte Carlo simulation agreement, and understanding the effect of hardware differences within the detector. We discuss the single photoelectron identification procedure and how we extract the single-photoelectron charge distribution using a deconvolution of the multiple-photoelectron charge distribution.

KEYWORDS: IceCube, single-photoelectron charge distribution, photomultiplier tubes, calibration

ARXIV EPRINT: [tbd](#)

Contents

1	Introduction	1
2	<u>Experimental setup</u>	1
2.1	<u>Single-photoelectron charge distributions</u>	4
2.2	Single-photoelectron charge distributions	5
2.2	IceCube datasets and software definitions	7
3	Extracting the SPE charge templates	8
3.1	Single photoelectron pulse selection	8
3.2	Characterizing the low-charge region	10
3.3	Fitting procedure	12
3.4	SPE charge template fit results	13
4	Discussion	15
4.1	Correlations between fit parameters and DOM hardware differences	15
4.2	Fitting parameters variation over time	18
4.3	Quantifying observable changes when modifying the PMT charge distributions	19
4.3.1	Model comparison	21
4.4	SPE charge templates for calibration	22
4.5	SPE charge templates in simulation	22
5	Conclusion	24

1 Introduction

This article discusses a method for determining the in-situ single-photoelectron (SPE) charge distributions of individual photomultiplier tubes (PMT) used in the IceCube neutrino detector. The SPE charge distribution refers to the charge probability density function of an individual PMT generated by the amplification of a pure sample of single photoelectrons. An accurate measurement of the individual SPE charge distribution is important for PMT calibration, since a change in the PMT gain corresponds to a proportional change in the extracted charge. Beyond this, a more accurate description of the individual SPE charge distributions in Monte Carlo (MC) simulation can also improve the overall data/MC agreement. The features extracted from the SPE charge distributions are also useful for examining hardware difference, such as the quantum efficiency, and assessing long term stability of the detector.

2 Experimental setup

The IceCube Neutrino Observatory [2, 3] (Fig. 1) is a cubic-kilometer-sized array of 5,160 photomultiplier tubes (PMTs) buried in the Antarctic ice sheet, designed to observe high-energy neutrinos interacting with the ice [4]. In 2011, the IceCube Collaboration completed the installation of 86 vertical strings of PMT modules, eight of which were arranged in a denser configuration known as the DeepCore sub-array [5]. Each string in IceCube contains 60 digital optical modules (DOMs), which contain a single PMT each, as well as all required electronics [6]. The primary 78 strings (excluding DeepCore) are spaced 125 m apart in a hexagonal grid, with the DOMs extending from 1450 m to

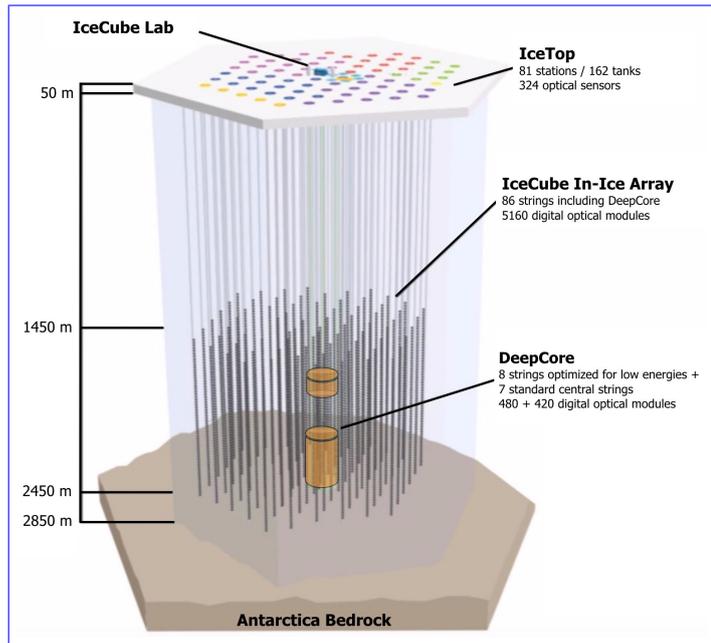


Figure 1. The IceCube Neutrino Observatory. From Ref. [1].

2450 m below the surface of the ice sheet. The additional DeepCore strings (79-86) are positioned between the centermost strings in the detector, reducing the horizontal DOM-to-DOM distance in this region to between 42 m and 72 m. The lower 50 DOMs on these strings are located in the deepest 350 m of the detector surrounded by the the cleanest ice [7], while the upper ten provide a cosmic ray veto extending down from 1900 m to 2000 m below the surface. Above the in-ice detectors, there exists a surface array, IceTop [8], consisting of 81 stations located just above the in-ice IceCube strings. The PMTs located in IceTop DOMs operate at a lower gain and the data from these PMTs was not included in the current analysis; however, the IceTop PMTs are calibrated to single photoelectron charge distribution in a similar way as the in-ice PMTs (see Sec. 5.1 in Ref. [8]).

Each DOM consists of a 0.5"-thick spherical glass pressure vessel that houses a single down-facing 10" PMT from Hamamatsu Photonics. The PMT is coupled to the glass housing with optical gel and is surrounded by a wire mesh to reduce the effect of the Earth's ambient magnetic field. The glass housing is transparent to wavelengths of 350 nm and above [9].

Of the 5,160 DOMs, 4,762 house a R7081-02 Hamamatsu Photonics PMT, sensitive to wavelengths ranging from 300 nm to 650 nm, with a peak quantum efficiency of 25% near 390 nm. These are classified as Standard Quantum Efficiency (Standard QE) DOMs. The remaining 398 DOMs are equipped with the Hamamatsu R7081-02MOD PMTs, which, having a peak quantum efficiency of 34% near 390 nm (36% higher efficiency than the Standard QE DOMs), are classified as High Quantum Efficiency (HQE) DOMs [5]. These DOMs are primarily located in DeepCore and on strings 36 and 43, as shown in the left side of Fig. 2.

The R7081-02 and R7081-02MOD PMTs have 10 dynode stages and are operated with a nominal gain of 10^7 and achieved with high voltages ranging from approximately 1215 ± 83 V and

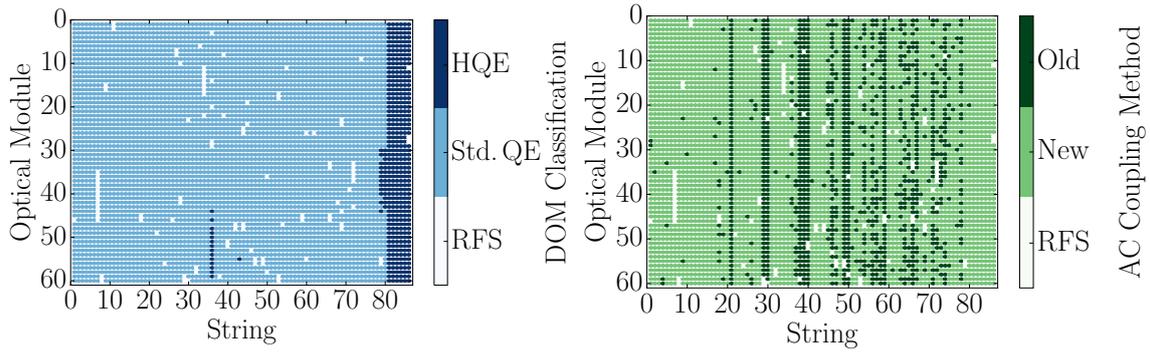


Figure 2. Left: A mapping of the HQE (dark blue) and Standard QE DOMs (light blue). Right: The version of AC coupling, old toroids (dark green) and new toroids (light green). DOMs that ~~have been were~~ removed from service (~~OTSRFS~~) for the IC86.2016 season are shown in white. ~~These are primarily DOMs that resulted in failures during deployment and failures during subsequent operation. Due to subsequent DOM failures, the number of RFS DOMs from IC86.2011 to IC86.2016 varies between 107 to 111.~~

1309 ± 72 V, respectively. A typical amplified single photoelectron generates a 5.2 ± 0.3 mV peak voltage after digitization with a full width at half maximum of 13 ± 1 ns. The PMTs ~~operate are operated~~ with the anodes at high voltage, so ~~the signal in order to remove the DC voltage from the signal, the PMT~~ is AC coupled to the amplifiers (front-end amplifiers). There are two versions of AC coupling ~~in the detectors employed in the PMTs~~, referred to as the *new* and *old toroids*, both of which use custom-designed ~~wideband bifilar wound 1:1 toroidal transformers~~¹. ~~The locations of DOMs with the different versions of AC-coupling are shown on the right side of Fig. 2~~ toroidal transformers. ~~The new toroids were designed with a larger ferrite core and more turns resulting in a droop time constant of $15\mu\text{s}$, ten times larger than the time constant of the old toroids.~~ The DOMs instrumented with the old toroids were ~~also~~ designed with an impedance of $43\ \Omega$, while the new toroids are $50\ \Omega$. ~~The toroidal transformer effectively acts as a high-pass filter with an approximately flat frequency response up to 100MHz. Single photoelectrons, measured at the output of the secondary winding, however, show percent-level shape differences between new and old toroids. The toroidal coupling method was chosen partial since it offers a higher level of reliability than capacitive coupling and has lower stored energy for the same frequency response [10]. Conventional AC-coupling high-voltage ceramic capacitors can also produce undesirable noise from leakage currents and are impractical given the signal droop and undershoot requirements [9]. The locations of DOMs with the different versions of AC-coupling are shown on the right side of Fig. 2.~~ All HQE DOMs are instrumented with the new toroids.

IceCube relies on two observables per DOM to reconstruct events: the total number of detected photons and their timing distribution. Both the timing and the number of photons are extracted from the digitized waveforms. This is accomplished by deconvolving the digitized waveforms ~~{H}~~ into ~~a series of scaled into a superimposition of~~ single photoelectron pulses (so-called pulse series), and

¹~~The toroidal transformer effectively acts as a high-pass filter with good signal fidelity at high frequencies and offers a higher level of reliability than capacitive coupling. Conventional AC-coupling high-voltage ceramic capacitors can also produce undesirable noise from leakage currents and are impractical given the signal droop and undershoot requirements [9].~~

the integral of the individual pulses divided by the load resistance defines the observed charge. It will often be expressed in units of PE, or photoelectrons, which further divides the measured charge by the charge of a single electron times the nominal gain.

When one or more photoelectrons produce a voltage at the anode sufficient to trigger the onboard discriminator, the signal acquisition process is triggered. The discriminator threshold is set to approximately 1.2 mV, or equivalently to ~ 0.23 PE, via a digital-to-analog converter (DAC). The signal is presented to four parallel channels for ~~digitization. Three channels pass through a 75 ns delay loop in order to capture the waveform leading up to the rising edge of the triggering pulse, and are then subject to different levels of amplification prior to being~~ analog amplification and digitization. The highest-gain channel has a nominal amplification of 16 and is most suitable for single photon detection, and is thus used in this analysis. This channel is digitized at 300 million samples per second (MSPS) for 128 samples (the readout time window of 427 ns) using a 10-bit Analog Transient Waveform Digitizer (ATWD). ~~The high-gain channel has a nominal amplification of 16 and is most suitable for single photon detection.~~ Two ATWD chips are present on the DOM Mainboard (MB) and alternate digitization between waveforms to remove dead time associated with the readout. ~~The signal to the fourth parallel channel is first shaped and amplified, then fed into a 10-bit fast analog-to-digital converter (fADC) operating at a sampling rate of 40 MSPS. Further detail regarding the description of the DOM electronics can be found in Refs. [6, 12].~~

~~This article discusses a method for determining the~~

2.1 Single-photoelectron charge distributions

~~The assessment of the in-situ individual PMT single-photoelectron charge distributions, which can be used to improve calibration and the overall detector description in Monte Carlo (MC) simulation. The SPE charge distribution refers to the charge probability density function of an individual PMT generated by the amplification of a pure sample of single photoelectrons. The measured shape of the SPE charge distributions is shown to be useful for examining hardware differences and assessing long term stability of the detector. This was recently~~ single-photoelectron charge distributions was made possible with the development of two pieces of software:

1. A specially-designed unbiased pulse selection developed to reduce the multiple photoelectron (MPE) contamination while accounting for other physical phenomena (e.g. late pulses, afterpulses, pre-pulses, and ~~baseline shifts~~waveform distortions) and software-related effects (e.g. pulse splitting). This is further described in Sec. 3.1.
2. A fitting procedure developed to separate the remaining MPE contamination from the SPE charge distribution by deconvolving the measured charged distribution. This is further described in Sec. 3.3.

By using in-situ data to determine the SPE charge distributions, we accurately represent the individual PMT response as a function of time, environmental conditions, software version and hardware differences, and realistic photocathode illumination conditions. This is beneficial since it also allows us to inspect the stability and long-term behavior of the individual DOMs, verify previous calibration, and correlate features with specific DOM hardware.

2.2 Single-photoelectron charge distributions

Ideally, a single photon produces a single photoelectron, which is then amplified by a known amount, and the measured charge ~~corresponds~~ is calibrated to correspond to 1 PE. However, there are many physical processes that create a spurious structure in the measured charge distributions. For example:

- **Statistical fluctuation due to cascade multiplication** [13]. At every stage of dynode amplification, the number of emitted electrons that make it to the next dynode is randomly distributed. This in turn causes a smearing in the measured charge after the gain stage of the PMT.
- **Photoelectron trajectory**. Some electrons may deviate from the favorable trajectory, reducing the number of secondaries produced at a dynode or the efficiency to collect them on the following dynode. This can occur at any stage, but it has the largest effect on the multiplication at the first dynode [14]. The trajectory of a photoelectron striking the first dynode will depend on many things, including where on the photocathode it was emitted, the uniformity of the electric field, the size and shape of the dynodes [13], and the ambient magnetic field [15, 16].
- **Late or delayed pulses**. A photoelectron can elastically or inelastically backscatter off the first dynode. The scattered electron can then be re-accelerated to the dynode, creating a second pulse. The difference in time between the initial pulse and the re-accelerated pulse in the R7081-02 PMT was previously measured to be up to 70 ns [9, 17]. Elastically backscattered photoelectrons will carry the full energy and are thus expected to produce similar charge to a non-backscattered photoelectron, albeit with a time offset. The mean measured charge of an inelastic backscattered photoelectron, by contrast, is expected to be smaller than a nominal photoelectron [18].
- **Afterpulses**. When photoelectrons or the secondary electrons produced during the electron cascade gain sufficient energy to ionize residual gas in the PMT, the resulting positively charged ionized gas will be accelerated in the electric field towards the photocathode. Upon impact with the photocathode, multiple electrons can be released from the photocathode, creating what is called an afterpulse. For the R7081-02 PMTs used in IceCube, the timescale for afterpulses was measured to occur from 0.3 to 11 μ s after the initial pulse, with the first prominent afterpulse peak occurring at approximately 600 ns [9]. The spread in the afterpulse time depends on the position of photocathode, the charge-to-mass ratio of the ion produced, and the electric potential distribution [19], whereas the size of the afterpulse is related to the momentum and species of the ionized gas and composition of the photocathode [20].
- **Pre-pulses**. If an incident photon passes through the photocathode without interaction and strikes ~~one of the dynodes~~ the first dynode, it can eject an electron that is only amplified by the subsequent stages, resulting in a lower measured charge (lower than the SPE pulse size by a factor of approximately 10 to 20). For the IceCube PMTs, the prepulses have been found to arrive approximately 30 ns before the signal from ~~other photoelectrons~~ photoelectrons emitted

from the photocathode. [The rate of pre-pulses was measured to be less than 1% of the SPE rate \[9\].](#)

- **MPE contamination.** When multiple photoelectrons arrive at the first dynodes within few nanoseconds of each other, they can be reconstructed by the software as a single MPE pulse.
- **Dark noise.** Photoelectron emission, not initiated from an external event, can be attributed to thermionic emission from the low work function photocathode and the dynodes, Cherenkov radiations initiated from radioactive decay within the DOM, and field emission from the electrodes. Dark noise originating from thermionic emission from the dynodes is shown in Ref. [21] to populate the low-charge region. [In the temperature range of interest for IceCube \(-40° to -20°\) the dark noise rate for the R7081-02 PMTs are approximately 350 Hz \[9\].](#)
- **Electronic noise.** This refers to the combined fluctuations caused by noise generated from the analog-frontend and the analog-to-digital converters (ATWDs and fADC). When integrated over a time window the resulting charge is generally small and centered around zero, thus only leading to a small broadening in the low charge region. The standard deviation of the electronic noise was found to be approximately ± 0.11 mV.

Beyond the physical phenomena above that modify the measured charge distribution, there is also a lower limit on the smallest charge that can be extracted. For IceCube, the discriminator only triggers for peak voltages above the threshold and subsequent pulses in the readout window are subject to a threshold defined in the software. This software threshold was set conservatively to avoid extracting pulses that originated from electronic noise. It can be modified to gain access to lower charge pulses and will be discussed in Sec. [3.2 at the expense of introducing more electronic noise into the charge distribution.](#)

The standard SPE charge distribution used for all DOMs in IceCube, known as the TA0003 distribution [9], models the above effects as the sum of an exponential plus a Gaussian. The TA0003 distribution is the average SPE charge distribution extracted from a lab measurement of 118 Hamamatsu R7081-02 PMTs. The measurement was performed in a -32°C freezer using a pulsed UV LED centered along the axis of the PMT, directly in front of the photocathode.

[Recently in 2013,](#) IceCube has made several lab measurements of the SPE charge distribution of R7081-02 PMTs using single photons generated from synchronized short duration laser pulses. The coincident charge distribution generated by the laser pulses was found to include a steeply falling low-charge component in the region below the discriminator threshold. To [improve the fit quality and](#) account for this, a new functional form including a second exponential was introduced. This form of the normalized charge probability distribution $f(q)_{\text{SPE}} = \text{Exp}_1 + \text{Exp}_2 + \text{Gaussian}$, is referred to as the *SPE charge template* in this article. Explicitly, it is:

$$f(q)_{\text{SPE}} = \frac{P_{e1}}{w_1} \cdot e^{-q/w_1} + \frac{P_{e2}}{w_2} \cdot e^{-q/w_2} + \frac{1 - P_{e1} - P_{e2}}{\sigma \sqrt{\pi/2} \cdot \text{Erfc}[-\mu/(\sigma\sqrt{2})]} \cdot e^{-\frac{(q-\mu)^2}{2\sigma^2}}, \quad (2.1)$$

where q represents the measured charge; w_1 and w_2 are the exponential decay widths; and μ , σ are the Gaussian mean and [width standard deviation \(SD\)](#), respectively. The coefficients P_{e1} , P_{e2} , and $1 - P_{e1} - P_{e2}$ correspond to the probability of a photoelectron contributing to each component of

the SPE template. The Erfc function used to normalize the Gaussian represents the complementary error function defined as $\frac{2}{\sqrt{\pi}} \int_x^\infty e^{-x^2} dx$. Eq. 2.1 is the assumed functional shape of the SPE charge distributions, and the components of Eq. 2.1 are determined in this article for all in-ice DOMs. IceCube has chosen to ~~defines~~ define 1 PE as the location of the Gaussian mean (μ) and calibrates the gain of the individual PMTs prior to the start of each season to meet this definition. Any overall bias in the total observed charge can be absorbed into an efficiency term, such as the quantum efficiency. This is valid since the linearity between the instantaneous total charge collected and the number of incident photons is satisfied up to ~ 2 V [10], or approximately 560 ~~PE~~ SPEs. That is, the average charge collected from N photons is N times the average charge of the SPE charge distribution, and the average charge of the SPE charge distribution is always a set fraction of the Gaussian mean.

2.2 IceCube datasets and software definitions

The amount of observed light depends on the local properties of the ice [7]. Short term climate variations from volcanoes and longer-term variations from atmospheric dust affect the optical properties of the ice, producing nearly horizontal layers. This layered structure affects how much light the DOMs ~~observes~~ observe, and, with it, the trigger rate. The largest contribution to the IceCube trigger rate comes from downward-going muons produced in cosmic ray-induced showers [22]. Cosmic ray muons stopping in the detector cause the individual trigger rates to decrease at lower depths.

If a DOM and its nearest or next-to-nearest neighbor observe a discriminator threshold crossing within a set time window, a *Hard Local Coincidence* (HLC) is initiated, and the corresponding waveforms are sampled and read out on the ~~three~~ ATWD channels. Thermionic emission induced dark noise can be present in the readout, however it is suppressed at lower temperatures and is unlikely to trigger an HLC event.

After waveform digitization, there is a correction applied to remove ~~measured baseline offsets~~ the DC baseline offset. Distortions to the waveform, such as from droop and undershoot ~~[9]~~ (see Ref. [23] for a technical description) introduced by the ~~toroidal transformer AC coupling~~ AC coupling, are compensated for in software during waveform calibration ~~by adding the expected~~. The area encompassed by the distortion of the waveform due to these effects is proportionally related to the charge that produced them, and is therefore commonly a problem for bright events or high frequency trains of photons. The expected distortion can be calculated if the input charge is known, and is compensated for by adding the determined reaction voltage of the distortion to the calibrated waveform. If the undershoot voltage drops below 0 ADC counts (outside of the minimum ADC range), the ADC values are zeroed and then compensated for once the waveform is above the minimum ADC input. ~~For each version of the AC coupling, scaled single photoelectron pulse shapes are then fit to the digitized waveforms using software referred to as~~

The digital waveforms are then deconvolved into a pulse series using software called "WaveDeform" (waveform unfolding process), ~~which determines the individual pulse time and charges and populates a pulse series.~~ [11]. The pulse series for a particular DOM corresponds to a list of single photoelectron charges and timestamps. WaveDeform is a fitting algorithm that determines the pulse series by fitting a superposition of single photoelectron basis functions to the the digitized waveforms. The basis functions, or SPE pulse templates, depend on the version of the AC-coupling

instrumented in the particular DOM. The pulse series, extracted from various datasets, represents the fundamental unit of data used in this analysis.

The pulse series used in this analysis come from two datasets:

1. The **MinBias-Event** dataset. This dataset preserves the full digital waveform readout of ~~randomly-triggered-randomly-selected~~ HLC events, collecting on average 1 ~~in every~~ 1000 HLC events. The largest contribution to this dataset comes from downward-going muons produced in cosmic-ray-induced showers. The average event ~~for this sample is consists of~~ approximately 26 PE distributed over an average of 16 ~~triggered-DOMs-DOMs that observed a discriminator crossing~~. The full digital waveform of these events allows us to extract the raw information about the individual pulses. This dataset will be used to measure the individual PMT charge distributions.
2. The **BeaconLaunch-Forced-Triggered (FT)** dataset. This dataset is populated with digitized waveforms that are initiated by the electronics (forced-triggered) of a channel that has not gone above the threshold. The forced triggered waveforms are typically used to monitor the individual DOM baselines and thus includes the full ATWD waveform readout. Since this dataset is forced-triggered, the majority of these waveforms represent electronic noise with minimal contamination from random accidental coincidence SPEs. This dataset will be used to examine the noise contribution to the charge distributions.

~~When using this dataset, the weight of every pulse is multiplied by a factor of 28.4 to account for the livetime difference between the MinBias dataset and the BeaconLaunch dataset. Weight, in this context, refers to the number of photons in the MinBias dataset proportional to one statistical photon in the BeaconLaunch dataset for which both datasets have the same equivalent livetime.~~

This analysis uses the full MinBias and BeaconLaunch-Event and FT datasets from IceCube seasons 2011 to 2016 [24], subsequently referred to as IC86.2011 to IC86.2016. Seasons in IceCube typically start in May of the labeled year and end approximately one year later. Calibration is performed before the start of each season.

3 Extracting the SPE charge templates

3.1 Single photoelectron pulse selection

The pulse selection is the method used to extract candidate, unbiased, single photoelectron pulses from ~~high-gain-highest-gain~~ ATWD channel while minimizing the MPE contamination. The ~~design of the~~ pulse selection was designed such that it avoids collecting afterpulses, does not include late pulses originating from the trigger pulse, accounts for the discriminator threshold, reduces the effect of signal droop and undershoot, and ~~gives-provides~~ sufficient statistics to perform a season-to-season measurement. An illustrative diagram of the pulse selection is shown in the left side of Fig. 3, while a description of the procedure is detailed below.

We restrict the pulse selection to only extract information from waveforms in which the trigger pulse does not exceed 10 mV (~ 2 PE) and no subsequent part of the waveform exceeds 20 mV

(~ 4 PE). This Here, since we are placing a limit on the input charge, this reduces the effect of the baseline undershoot due to the AC coupling or other artifacts from large pulses.

In order to trigger a DOM, the input to the front-end amplifiers must exceed the discriminator threshold. To avoid the selection bias of the discriminator trigger (i.e. only selecting pulses greater than the discriminator threshold), we ignore the trigger pulse as well as the entire first 100 ns of the time window. This is shown as region A in Fig. 3 (left). Ignoring the first 100 ns removes late pulses that could be attributed to the triggering pulse, which occurs approximately 4% of the time [9].

To ensure we are not accepting afterpulses into the selection (recall that the first prominent afterpulse peak occurs at approximately 600 ns), we also enforce the constraint that the pulse of interest (POI) is within the first 375 ns of the ATWD readout time window. This also allows us to examine the waveform up to 50 ns after the POI (the full ATWD readout window is 427 ns). In the vicinity of the POI, we ensure that WaveDeform did not reconstruct any pulses up to 50 ns prior to the POI, or 100 to 150 ns after the POI (the light gray region of these regions are labelled as B and D in Fig. 3 (left)). This latter constraint is to reduce the probability of accidentally splitting a late

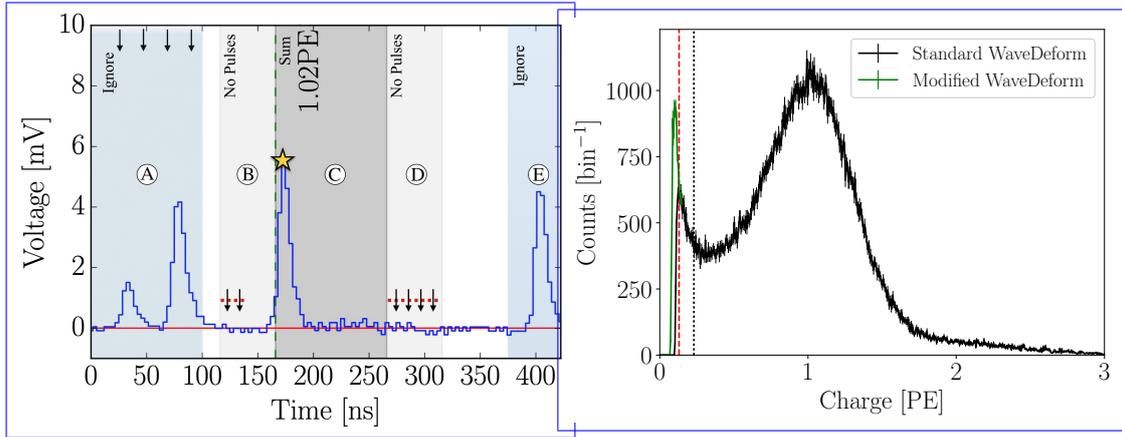


Figure 3. Left: An illustrative diagram of the pulse selection criteria for selecting a high-purity and unbiased sample of single photoelectrons. An example digitized ATWD waveform of data is shown in blue and the baseline is shown as a solid red line. The pulse of interest is identified with a yellow star. This example waveform was triggered by a small pulse at 25 ns (recall that the delay board allows us to examine the waveform just prior to the trigger pulse), followed by a potential late pulse at 70 ns. At 400 ns, we see a pulse in the region susceptible to afterpulses. Waveform voltage checks are illustrated with arrows, and various time windows described in the text are drawn with semi-opaque regions. The pulse of interest (POI) is reported to have a charge of 1.02 PE, given by WaveDeform, and would pass the pulse selection criteria. Right: The collected-measured charge distribution resulting from the pulse selection for string 1, optical module 1 (DOM 1,1), from the MinBias-Event dataset collected from IC86.2011 to IC86.2016 that pass the pulse selection. The red dashed line and (black dotted line indicate 0.15 PE and 0.25 PE respectively data points with statistical error bars). The As described in the text, the pulse selection access-charges-is able to extract charge below the discriminator threshold of 0.23 PE (black dotted line). The fall-off-threshold shown in charge-around-the black data points below 0.13 PE (red dashed line) is due to the software-defined threshold-from-termination condition in WaveDeform. After setting to termination condition to a lower value (modified WaveDeform), the charge distribution is extended to lower charges, as exemplified by the green data points.

pulse in the summation window.

If a ~~pulse-POI~~ is reconstructed between 100 and 375 ns after the start of the waveform and the voltage criteria ~~above~~ are met, it is accepted as a candidate photoelectron and several checks are performed on the waveform prior to and after the ~~pulsePOI~~. The first check is to ensure that the waveform is near the baseline just before the rising edge of the POI. This is accomplished by ensuring that the waveform does not exceed 1 mV, 50 to 20 ns prior to the POI, and eliminates cases where the POI is a late pulse. We also ensure the waveform returns to the baseline by checking that no ADC measurement exceeds 1 mV, 100 to 150 ns after the POI. These constraints are illustrated as the horizontal red dotted lines and black arrows in ~~regions B and D in~~ the left side of Fig. 3.

If all the above criteria are met, we sum the reconstructed charges ~~in the pulse series~~ from the POI time, given by WaveDeform, to +100 ns (~~the dark gray area region C~~ in Fig. 3 (left)). This ensures that ~~any-all~~ nearby pulses are either fully separated or fully added. This ~~is important summation is critical~~, since WaveDeform may occasionally split ~~an-a true~~ SPE pulse into multiple smaller pulses, therefore ~~it is always critical to we must always~~ perform a summation of the charge within a time window ~~-The to produce a meaningful charge distribution. Consequently, the~~ 100 ns summation ~~also means (region C) also implies~~ that the pulse selection will occasionally accept MPE events. We chose 100 ns window for the summation to ~~ensure-be sufficiently large~~ that we collect the charge of ~~the-a~~ late pulse (recall that late pulses were measured up to 70 ns after the main pulse), should it be there, while minimizing the MPE contamination. ~~We-After running the pulse selection, we~~ estimate that there is on average a 6.5% probability of the summation time window includes ~~a MPE-pulsetwo or more photons~~.

3.2 Characterizing the low-charge region

This analysis aims to describe the ~~full-SPE-charge-distribution-entire charge probability distribution down to zero charge~~ for each DOM. This is required by the IceCube simulation. However, we cannot extract charge to arbitrary low ~~PE-values~~ before electronic noise ~~starts dominating~~. ~~The aim of this section is to describe how we extract information in the low-charge region (below 0.25 PE) to guide the full fit begins to dominate~~. Fig. 3 (right) shows the charge distributions ~~of the selected pulses that pass the single photoelectron from the Event dataset as black data points after the~~ pulse selection for string 1, optical module 1, DOM(1,1). ~~In the low-charge region-By ignoring the first 100 ns of the ATWD time window, we see a-second-threshold-at-approximately-that we are capable of extracting charge below the discriminator threshold (vertical black dashed line).~~

~~The threshold observed below 0.13 PE, i.e.-the-charge-distribution-terminates. This threshold arises from~~ is due to the software threshold mentioned in Sec. 2.1. The threshold is a result ~~of the settings employed within WaveDeform. These settings include~~ a termination condition ~~in WaveDeform, in which the pulses that are smaller than predefined criteria are rejected. The threshold was set to avoid electronic noise being interpreted as PMT pulses and contaminating the low-charge region on the SPE pulse template fitting algorithm that monitors the gradient of the least-squares residual in the fit to the digitized waveforms. When the improvement to the fit, per PE, of allowing one more non-zero pulse drops below the value of the termination condition, the algorithm will terminate. By reducing the value of the termination condition setting, WaveDeform is slower but will produce a better fit to the data and fit and include smaller pulses. The extension~~

to the charge distribution is shown as the green data points in Fig. 3 (right). Reducing this value, however, will also increase the electronic noise contamination. An assessment of this follows.

The steeply falling component of the region from above the WaveDeform threshold and below the discriminator (0.13 PE to 0.250.23 PE) is in agreement with the laser measurements mentioned in Sec. 2.1 and emphasizes the importance of collecting data below the discriminator threshold. This section will assess the noise contribution to this region and examine the effect on. Since small pulses below the DOM's discriminator threshold will be recorded in events with multiple photoelectrons, it is important that the SPE charge distribution accounts for this shape. Exp₁ was specifically introduced into Eq. 2.1 to account for this component. It was an empirical choice to use an exponential to represent this region of the charge distribution and noise contribution by lowering the WaveDeform threshold.

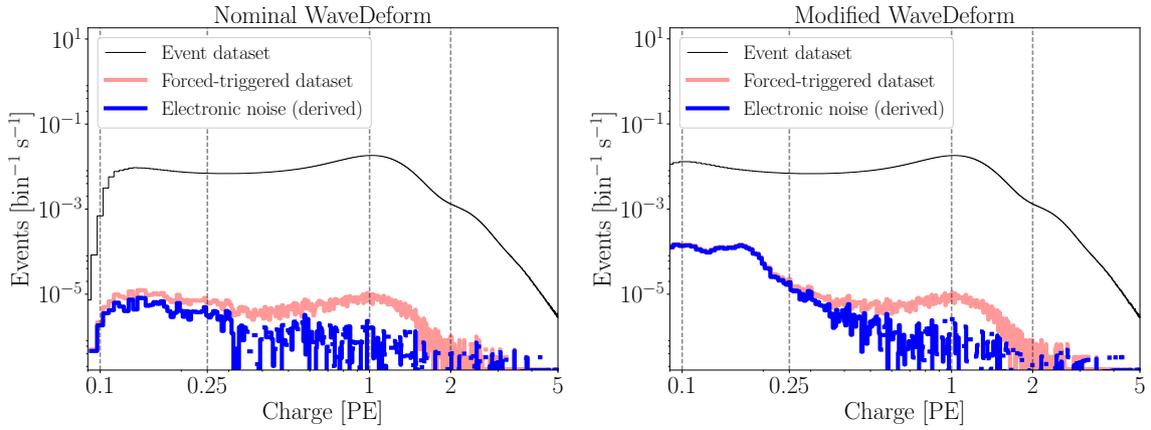


Figure 4. The cumulative charge distributions of all DOMs for the MinBias-Event (ME) and BeaconLaunch Forced-triggered (BFT) datasets summed over all seasons. The blue histogram shows the derived contribution from electronic noise. This was found by subtracting the normalized MinBias-Event dataset (normalized such that the rate between E and FT are the same 1PE) from the BeaconLaunch-FT dataset: $(B-FT - ME \times (BFT)_{1PE} / (ME)_{1PE})$. Left: The charge distributions for the standard WaveDeform settings. Right: The charge distributions for the modified WaveDeform settings.

Fig. 4 (left) shows the charge distributions for the MinBias summed over all DOMs for the Event (black) and the BeaconLaunch-FT (red) datasets using the default settings of WaveDeform (standard WaveDeform). As mentioned in Sec. 2.2, occasionally a photoelectron will be coincident with the forced BeaconLaunch-FT time window. These charges populate a SPE charge distribution. Subtracting the shape of the MinBias charge distribution from the BeaconLaunch dataset Event dataset charge distribution – which is dominated by single photoelectrons – from the FT dataset, yields an estimate of the amount of electronic noise contamination (blue). The bin in the MinBias Event data with the lowest signal-to-noise ratio (SNR) above 0.1 PE was found to have a SNR of 744.7. The SNR for the full distribution was found to be 1.98×10^5 .

Fig. 4 (right) shows the same data after lowering the WaveDeform threshold (modified WaveDeform), and is found to have SNR of 57.9 in the bin with the largest contamination and the total SNR

was found to be 0.69×10^5 .

~~The modified WaveDeform datasets show a minimal increase in the contribution of noise to While the noise is observed to increase (as expected) with the modified WaveDeform, the low-charge region. From this, however, we are able to extract charge information down to approximately 0.10 PE and improve the overall description of the charge distribution below the discriminator. This will help constrain the values of the steeply falling exponential, defined with Exp_1 contamination level is still considered minimal (below 2% in any bin).~~

3.3 Fitting procedure

We would now like to fit the charge distribution to extract the SPE charge templates (the components of Eq. 2.1) for all DOMs.

Contamination from two-photon events is suppressed by the pulse selection, but can not be entirely avoided. To minimize potential biases by the charge entries resulting from two photons, the one and two photon contribution to the charge distributions is fitted at the same time, using something we call a convolutional fitter. It assumes that the charge distribution resulting from two photons is the SPE charge distribution convolved with itself [25]. In each step of the minimizer the convolution is updated given the current set of SPE parameters to be evaluated and the relative one and two photon contributions is determined.

We do not ~~account fit~~ for the three-photon contribution, which is justified by the lack of statistics in the 3 PE region as well as the significant rate difference between the 1 PE and 2 PE region, as shown in Fig. 3 (right).

~~Pulses that fall below the WaveDeform threshold and are not reconstructed contribute to an inefficiency in the individual DOMs. That is, the shape below the WaveDeform software threshold does not have a significant impact, but the relative area of the SPE charge template below compared to above this threshold changes the efficiency of the DOM. This analysis assumes the same shape of Although the pulse selection and the steeply falling exponential component (modification to WaveDeform allow us to probe the charge distribution below the discriminator, there is insufficient data to accurately fit Exp_1 to each DOM independently. Rather, we determine the value of Exp_1) using the aggregate of all data together, and use that result for Exp_1 in all subsequent fits.~~

~~The motivation to not fit for Exp_1 independently for all DOMs in the detector to avoid large fluctuations in the DOM-to-DOM efficiencies. The modified WaveDeform data will strictly be used to determine the is as follows. Pulses that fall below the WaveDeform threshold do not contribute to the pulse series. This is equivalent to a efficiency factor for DOM in question. Having large variations in the Exp_1 component will in turn cause large variation in the individual DOM efficiencies. Rather, setting all DOMs to have the same Exp_1 component. Specifically, using improves the overall fit while reducing the DOM-to-DOM efficiency differences. In IceCube analyses, a global efficiency systematic uncertainty accounts for this.~~

~~Using the aggregate of the entire ensemble of DOMs with the modified WaveDeform datasetdatasets, we background-subtract the BeaconLaunch FT distribution from the MinBias data, Event dataset (removing the electronic noise), and fit the resulting distribution to determine the components of Eq. 2.1, and use only the measured. The determined shape and normalization of Exp_1 in all subsequent standard WaveDeformfits is then used in all individual DOM fits using the standard WaveDeform.~~

Upon fitting the standard WaveDeform Event dataset with the determined values for Exp_1 , the residual of each fit is calculated by measuring the percentage difference between the fit and the data. By averaging the residuals over all the DOMs (shown in Fig. 5), a correction function is generated and will be used as a global additive factor for all SPE charge templates to account for the difference between the chosen model (Eq. 2.1) and the actual data. All SPE charge templates include the residual correction function in Fig. 5.


As described in Sec. 2.1, the Gaussian mean (μ) is used to determine the gain setting for each PMT. Therefore, it is particularly important that the fit quality in the peak region accurately describes the data. While fitting to the full charge distribution improves the overall fit agreement, the mismatch between the chosen functional form (Eq. 2.1) and a true SPE charge distribution can cause the Gaussian component to pull away from its ideal location. To compensate for this, the fitting algorithm prioritizes fitting to the data around the Gaussian mean. This is accomplished by first fitting to the full distribution to get an estimate of the Gaussian mean location (to within 1%). Then, the data in the region ± 0.15 PE around the original estimated Gaussian mean is weighted to have a higher impact on the fit, and the distribution is re-fitted. The re-fitting amounts to a percent level change in the Gaussian mean location and the chosen region around the original estimate of the Gaussian mean was found not to produce a significant bias.

Upon fitting the MinBias dataset with the predetermined values for Exp_1 , the residual of each fit is calculated by measuring the percentage difference between the fit and the data. The average residual is then used as a global scaling factor for all SPE charge templates to account for the difference between the chosen model (Eq. 2.1) and the actual data.

3.4 SPE charge template fit results

We now present the results of the fits and describe the correlations of the fit parameters with hardware differences, and time variations in the next section. Using the background-subtracted modified WaveDeform By subtracting the modified WaveDeform electronic noise spectrum (shown in Fig. 4) from the Event dataset, the Exp_1 component was determined by fitting the aggregate distribution from 0.1 PE to 3.5 PE. The result of the fit yielded $P_{e1} = 0.186 \pm 0.041$ and $w_1 = 0.027 \pm 0.002$ PE. This shape of Exp_1 , with a Pearson's correlation coefficient of -0.895. Determining the shape and normalization was the sole purpose of using the modified WaveDeform. All subsequent discussion relates to the standard WaveDeform datasets. The determined values for Exp_1 is are now used to describe the low-PE charge region for all subsequent standard WaveDeform fits.

Using the MinBias-Event dataset with the measured values of Exp_1 , the SPE charge templates are extracted for every DOM, separately for each IceCube season from IC86.2011 to IC86.2016. The fit range for Exp_2 and the

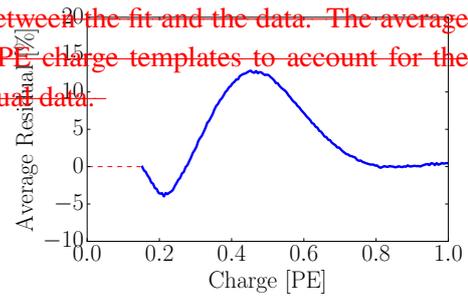

The extracted residual in blue, comparing the result of the convolutional fit to the data, averaged over all DOMs. The dashed red line indicates the region where we do not have sufficient data and therefore set the residual to 0% (i.e. no correction will be applied in this region).

Figure 5. The extracted residual correction in blue, comparing the result of the convolutional fit to the data, averaged over all DOMs. The dashed red line indicates the region where we do not have sufficient data and therefore set the residual to 0% (i.e. no correction will be applied in this region).

Gaussian components is selected to be between 0.15 PE and 3.5 PE. An average fit was also performed on the ~~cumulative~~ charge distribution, in which all the data for a given DOM was summed ~~together over all seasons~~ (labeled as "AVG").

~~All the DOMs with "failed fits" are not included in this analysis. A~~ An SPE charge template for a particular DOM is classified as having a ~~failed fit if it does not pass~~ "failed fit" if it is flagged by one of the validity checks ~~on the data requirements (e. g. the number of valid pulses) or~~. The validity checks ensure that there is sufficient data extracted from the pulse selection and that the fit was successful, as well as goodness of fit. ~~Over the seasons considered between 107 and 111 DOMs have been excluded from service and represent the majority of the failed fits~~ check on the reduced χ^2 . The majority of the failed fits, approximately 95%, are due to DOMs which have been removed from service (see Fig. 2). The remaining ~~6 DOMs that failed the AVG fits are known to have various issues~~ failed fits were found to be associated with DOMs that have known issues associated with their charge collection. All the DOMs with failed fits are not included in this analysis. In the ~~IceCube MC simulation chain, these DOMs are assigned~~ simulation, the average SPE charge template is assigned to these DOMs.

We can divide the DOMs into ~~subset of~~ subsets with the following hardware differences: ~~the~~

1. HQE DOMs with the new toroids, ~~the~~
2. Standard QE DOMs with the new toroids, ~~and the~~
3. ~~and~~ Standard QE DOMs with the old toroids.

The mean value and standard error of the ~~mean of the~~ IC86.AVG fit parameters, ~~excluding Exp₁~~, for the subset of hardware differences are listed in Table 1. The residual, averaged over all DOMs, from 0 to 1 PE is shown in Fig. 5.

Hardware Configuration	Exp ₂ Prob. (P_{e1})	Exp ₂ Width (w_2)	Gaus. Prob. ($1-P_{e1}-P_{e2}-P_{e3}$)	Gaus. Mean (μ)	Gaus. Width SD (σ)
HQE / New Toroid	0.243 0.245 ± 0.002	0.354 0.358 ± 0.004	0.570 0.569 ± 0.002	1.0148 1.0163 ± 0.0011	0.312 0.311 ± 0.002
NQE / New Toroids	0.210 0.211 ± 0.001	0.344 0.348 ± 0.001	0.604 0.602 ± 0.001	1.0183 1.0198 ± 0.0004	0.316 0.315 ± 0.001
NQE / Old Toroids	0.206 0.207 ± 0.001	0.377 0.381 ± 0.003	0.608 0.607 ± 0.001	1.0030 1.0044 ± 0.0008	0.294 0.293 ± 0.001

Table 1. The ~~average values and standard error~~ measured mean of each fit parameter ~~and the standard error of the mean~~ for the subset of hardware configurations listed in the first column. ~~The fitted parameters for Exp₁, determined at the beginning of this section, are: $P_{e1} = 0.186 \pm 0.041$ and $w_1 = 0.027 \pm 0.002$ PE.~~

An example fit is shown in Fig. 6 for the ~~cumulative~~ MinBias-Event dataset charge distribution for DOM (1,1). The collected charge distribution is shown in the black histogram, while the fit to the data is shown as the red line. The extracted SPE charge template from the fit is

shown in blue. Both the fit [result](#) and extracted SPE charge template [have been scaled by shown here incorporate](#) the average residual [shown found](#) in Fig. 5.

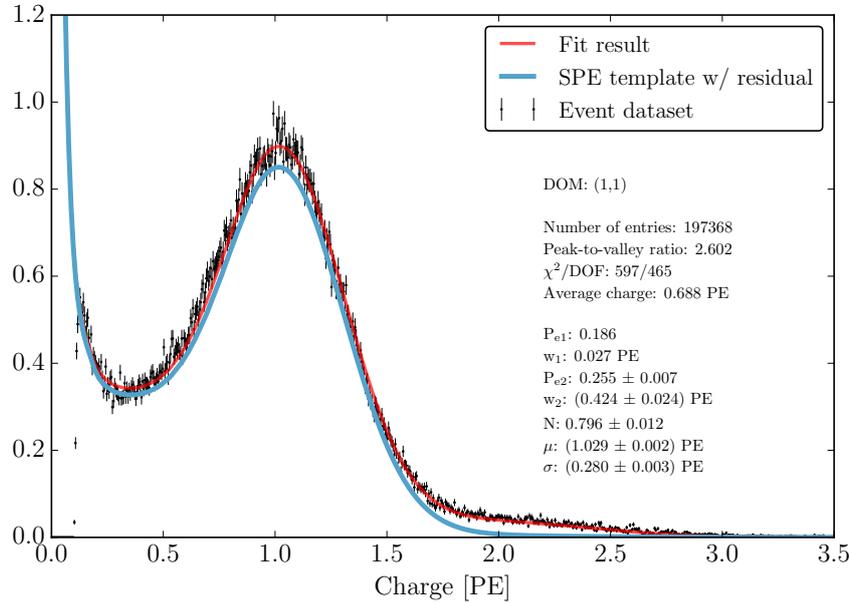


Figure 6. [An example-The result of the convolution fit \(red\)](#) for DOM(1,1) using the [MinBias-Event dataset \(black histogram data points with statistical uncertainties\)](#), including [all data from seasons IC86.2011 to IC86.2016](#). The [result of the convolution fit, which includes the 2 PE contribution, is shown as a solid red line and the extracted SPE charge template from the fit result is shown in blue](#). For both the convolution fit and the SPE charge template, the curves include the correction from the average residual shown in Fig. 5. [Here As discussed in Sec. 3.3, \$P_{e1} = 0.186\$ and \$w_1 = 0.027\$ PE are fixed for the individual DOM fits. The difference between the fit result and the SPE charge template is the 2PE contamination. The 2PE contribution is defined as discussed convolution of the SPE charge template with itself, and the SPE charge template is non-zero at low charges, the end of Sec. 3.2 2PE contribution is non-zero at low charges.](#)

4 Discussion

4.1 Correlations between fit parameters and DOM hardware differences

It is evident from the data in Table 1 that the average shape of the SPE charge templates depends on the DOM hardware. These differences can also be seen in the measured peak-to-valley ratios and average charge of the SPE charge template (see Fig. 7). [The peak-to-valley ratio is defined as the ratio between the maximum in the SPE charge template near the SPE peak divided by the minimum found near the discriminator.](#)

When we examine the subset of DOMs instrumented with the new toroids, the average HQE DOM were found to have a $20.215.85 \pm 0.60.04\%$ larger P_{e2} component and $4.75.56 \pm 0.40.01\%$ smaller Gaussian widthnorm. Consequently, the average HQE peak-to-valley ratio is measured to be $2.2552.25 \pm 0.012$, ~~corresponding to $13.670.01$, or $13.68 \pm 0.010.02\%$~~ lower than the average for Standard QE DOMs. Also, ~~interestingly~~, the average charge of the average HQE DOM was found to be $3.173.177 \pm 0.010.005\%$ lower than that of the Standard QE DOMs. The average charge is calculated by integrating over the full SPE charge template including the residual correction. The values shown in Fig. 7 (right) are found to be below 1 PE due to the low-PE contribution from Exp₁ and Exp₂, whose physical description can be found in Sec. 2.1.

IceCube compensates for the change in the mean measured charge in simulation, by increasing the HQE DOM efficiency by the equivalent amount. This ensures that the total amount of charge collected by the HQE DOMs remains the same prior to, and after, inserting the SPE charge templates into simulation.

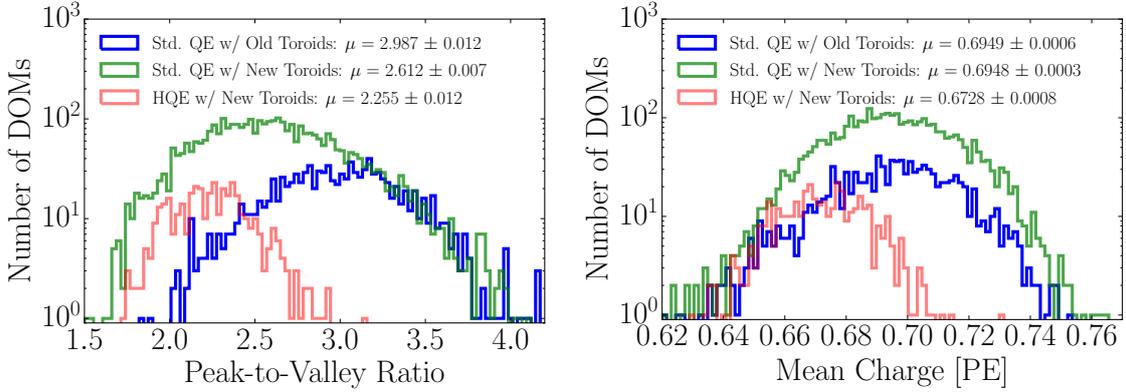


Figure 7. Comparison between the R7081-02MOD HQE DOMs and standard R7081-02 DOMs. Left: The peak-to-valley ratio for the two subsets of quantum efficiencies. Right: The average charge of the individual DOM SPE charge templates.

Similarly, using only the subset of Standard QE DOMs, the SPE charge templates ~~comparing the method of AC coupling~~ were found to have measurably different shapes when comparing the different methods of AC coupling. The average Gaussian width-standard deviation for the DOMs instrumented with the old toroids were found to be $8.16.99 \pm 0.10.01\%$ narrower, albeit with a very

similar probability of the photoelectron populating the Gaussian component. With these differences, we find a peak-to-valley ratio of 2.612 ± 0.007 for the new toroid DOMs and 2.987 ± 0.012 for the old toroid DOMs. The average Gaussian mean of the fit for the DOMs with the old toroids was also found to be $1.511 \pm 0.002\%$ lower than those with the new toroids. This corresponds proportionally to a change in the expected gain. The difference in the average charge, however, between these two hardware configurations is very similar, $0.004 \pm 0.003\%$.

Although the DOMs instrumented with the old toroids were deployed into the ice earlier than those with the new toroids, the differences above remain when examining individual deployment years; therefore, the shape differences are not attributed to the change in the DOM behavior over time. However, the DOMs with the old toroids were the first PMTs to be manufactured by Hamamatsu. A gradual change of the fit parameters was observed when ordering the PMTs according to their PMT serial number (i.e. their manufacturing order). Fig. 8 shows the change in the measured peak-to-valley ratio as a function of PMT serial number for the standard QE DOMs (blue) and HQE PMTs (red). Here, each data point represents a single PMT and the blue (red) data points indicate a PMT instrumented with the new (old) toroid. This is compelling evidence that the observed differences between the new and old toroids is due to a change in the PMT production procedure rather than version of AC coupling.

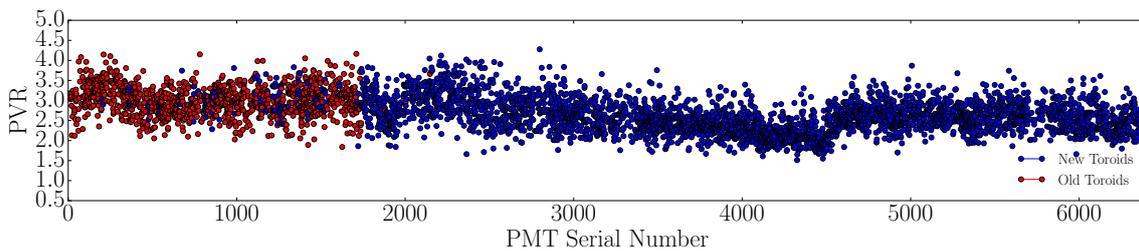


Figure 8. The measured peak-to-valley ratio for the standard QE PMTs ordered by PMT serial number. The red data points indicate a PMT instrumented with an old toroid, whereas new toroids are indicated by the blue data points.

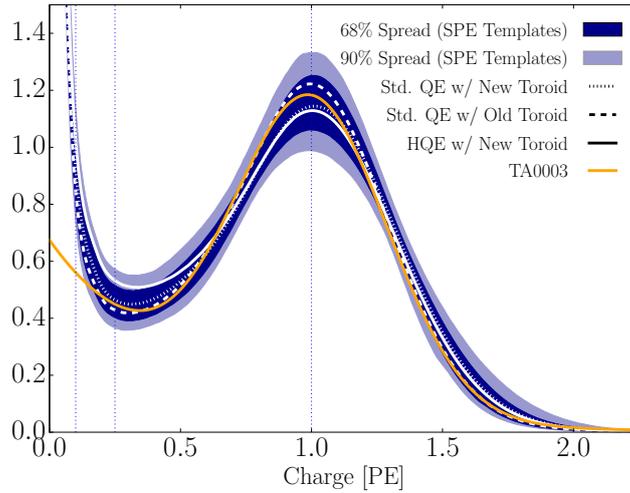


Figure 9. The inner (outer) dark blue region shows the 68% (90%) ~~confidence interval defined by the measured spread in the extracted SPE charge templates of all DOMs in the detector for a given charge.~~ Superimposed are the average SPE charge templates for the variety of hardware configurations shown in white. The TA0003 distribution, for comparison, is shown in orange. All curves have been normalized such that the area above 0.25 PE is the same.

Fig. 9 illustrates the average shape differences in the extracted SPE charge templates between the HQE DOM with the new toroids (solid white line), Standard QE with the new toroids (dotted white line), Standard QE with the old toroids (dashed white line), compared to the spread in the measured SPE charge templates for all DOMs in the detector (dark blue contours). The figure also shows how the previous default SPE charge distribution, the TA0003 distribution, compares to this recent measurement. All curves in this figure have been normalized such that the area above 0.25 PE is the same. The observable shape differences from the TA0003 are attributed to a better understanding of the low-charge region, the difference in functional form (described in Section 2.1), and the fact that the SPE charge templates were generated using a realistic photocathode illumination.

4.2 Fitting parameters variation over time

The SPE charge templates were also extracted for each IceCube season independently (IC86.2011 to IC86.2016), in order to investigate the time dependence of the fit parameters. The data was broken up into IceCube seasons

rather than years, since calibration to remove gain drift is performed at the beginning of each IceCube season.

For every DOM in the detector, the change over time of each fit parameter (excluding Exp_1 , since it was held fixed for this analysis) was calculated. Fig. 10 shows the change in a given fit parameter, relative to the mean value, per year IceCube season. The measured distributions were found to be consistent with statistically scrambling the yearly measurements. The average of each fit parameters randomly scrambling the order of each measurement. Greater than 96% of DOMs are found to deviate less than 0.1%, which is have less than 1.0% change per year in the measured location of the Gaussian mean, in agreement with the stability checks performed in Ref. [10]. This observation holds for the individual subset subsets of DOMs with different hardware configurations as well.

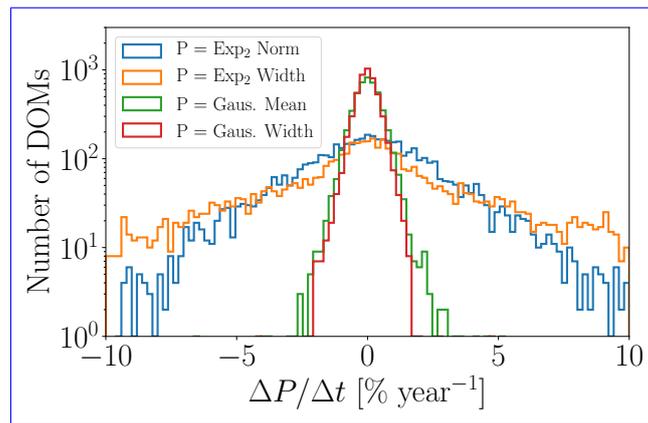


Figure 10. The change in the individual DOM fitted parameters over time, represented as percentage deviation from IceCube season IC86.2011 to IC86.2016. The histogram represents the mean fit rate of change, per IceCube season, of the fitted parameter value labelled in the legend.

4.3 Quantifying observable changes when modifying the PMT charge distributions

Changing In this section we investigate the extent to which changes to the SPE charge templates impact quantities such as the trigger fraction above our discriminator threshold or the measured charge over threshold, since these quantities are used in the analysis of IceCube physics events. If the choice of template has a significant impact on high-level physics results reported by IceCube, it would be a serious concern. Thus we explore the effect of changing the assumed gain response in simulation. The change has different implications depending on the typical illumination level

present in different ~~analyses.~~ ~~These differences are outlined in the following discussion~~ physics analyses. Therefore we explore the effect of the templates in three illumination regimes: dim, semi-bright, and bright illumination.

The PMT response function is described by a combination of a "bare" efficiency, η_0 , and a normalized charge response function, $f(q)$. The bare efficiency represents the fraction of arriving photons that result in any nonzero charge response, including those below the discriminator threshold. The normalization condition is:

$$\int_0^{\infty} f(q) dq = 1. \quad (4.1)$$

Generally, $f(q)$ and η_0 have to be adjusted together to maintain agreement with a quantity known from lab or in-ice measurements, such as the predicted number of pulses above threshold for a dim source.

Dim source measurements Where light levels are low enough, the low occupancy ensures that sub-discriminator pulses do not contribute to any observed charge as they do not satisfy the trigger threshold. Given some independent way of knowing the number of arriving photons, a lab or in-ice measurement determines the trigger fraction above threshold $\eta_{0.25}$ and/or the average charge over threshold $Q_{0.25}$, either of which can be used to constrain the model as follows:

$$\eta_{0.25} = \eta_0 \int_{0.23q_{pk}}^{\infty} f(q) dq \quad (4.2)$$

$$Q_{0.25} = \eta_0 \int_{0.23q_{pk}}^{\infty} q f(q) dq \quad (4.3)$$

Here, the discriminator threshold is assumed to be 0.25 times the peak position q_{pk} . It is also useful to multiply observed charges by q_{pk} , since we set each PMT gain by such a reference, and then a measurement constraint would be stated in terms of $Q_{0.25}/q_{pk}$.

Semi-bright source measurements For semi-bright sources, pulses that arrive after the readout time window is opened are not subject to the discriminator threshold. WaveDeform introduces a software termination condition at ~ 0.13 PE (described at the end of Section 3.1). The average charge

of an individual pulse that arrives within the time window is:

$$Q_{0.100.13} = \eta_0 \int_{0.10q_{pk}}^{0.13q_{pk}} q f(q) dq \quad (4.4)$$

Bright source measurements For light levels that are large (e.g. a cosmic ray muon passing near the photocathode), the trigger is satisfied regardless of the response to individual photons, and the total charge per arriving photon therefore includes contributions below both the discriminator and the WaveDeform thresholds:

$$Q_0 = \eta_0 \int_0^{\infty} q f(q) dq \quad (4.5)$$

As such, the total charge is directly proportional to the average charge of the SPE charge template.

4.3.1 Model comparison

A natural question to ask is whether or not a change in $f(q)$ would cause observable changes in the bright-to-dim ratios. That is, when we change the SPE charge distribution in simulation, should we expect the charge collected by bright events compared to dim events to change? When the charge distribution model is changed in a way that preserves agreement with the measured $\eta_{0.25}$ or $Q_{0.25}/q_{pk}$, i.e. η_0 is adjusted properly for changes in $f(q)$, the physical effect can be summarized by the change in the bright-to-dim ratios $Q_0/Q_{0.25}$, and $Q_0/Q_{0.100.13}$. Conveniently, these ratios depend only on the shape of $f(q)$. Table 2 compares these ratios in terms of the TA0003 charge distribution and the SPE charge templates described here. It is shown that there are sub-percent level differences in the physically-observable bright-to-dim ratios. The largest difference in the shape between the SPE charge templates and the TA0003 distribution is in the low-charge region, particularly below ~ 0.10 PE. Charge from this region can only inflate bright events. That is, these pulses are too small to trigger the discriminator or be reconstructed by WaveDeform, ~~however~~ but they can reside on top of other pulses, inflating them. Since these pulses by definition contain little charge, they do not tend to inflate the measured charge by a noticeable amount, as shown by the $Q_0/Q_{0.25-0.23}$ measurements in Table 2.

Model	Detector	$Q_0/Q_{0.25}Q_{0.23}$	$Q_0/Q_{0.10}Q_{0.13}$	$Q_{0.25}Q_{0.23}/Q_{0.25}Q_{0.23}$
TA0003	All DOMs	1.017 ± 0.014	1.003 ± 0.005	1.050 ± 0.017
SPE Templates	HQE + New Toroids	1.022 ± 0.002	1.004 ± 0.001	1.050 ± 0.017
SPE Templates	NQE-Std. QE + New Toroids	1.019 ± 0.002	1.004 ± 0.001	1.034 ± 0.018
SPE Templates	NQE-Std. QE + Old Toroids	1.017 ± 0.002	1.003 ± 0.001	1.048 ± 0.023

Table 2. The distribution in bright-to-dim ratios for the previous charge distribution (TA0003) and the individual DOM SPE charge templates for the IceCube and DeepCore detectors. The uncertainty reported represents the standard deviation of the distribution of the calculated quantity.

4.4 SPE charge templates for calibration

The gain setting on each PMT is calibrated prior to the beginning of each season such that the Gaussian mean of the charge distribution corresponds to a gain of 10^7 , or equivalently 1 PE. This gain calibration method, run directly on the DOMs, uses waveform integration for charge determination instead of WaveDeform unfolding, resulting in a small systematic shift in gain. This systematic shift was determined for every PMT. The mean shift obtained over all DOM was found to be $1.47 \pm 0.04\%$ with a standard deviation of 2.62% , corresponding to an overestimation of the measured charge in the detector.

The correction to the systematic shift in the measured charge can be implemented retroactively by dividing the reported charge from WaveDeform by the corresponding offset for a given DOM. Alternatively, we can account for this by simply inserting SPE charge templates, measured in this analysis, into simulation such that the corresponding systematic shift is also ~~modelled~~ modeled in simulation. This will be performed in the following subsection.

4.5 SPE charge templates in simulation

To model the IceCube instrument, ~~we must implement~~ the PMT response ~~in is~~ described in the simulation. The IceCube MC-simulation chain assigns a charge to every photoelectron generated at the surface of the photocathode. The charge is determined by sampling from a normalized SPE charge distribution probability density function (PDF). A comparison to data between describing the SPE charge distribution PDF using the SPE charge templates and the TA0003 distribution follows.

Two simulation sets consisting of Monte Carlo simulation datasets were produced, one using the SPE charge templates to describe the charge distribution for every DOM in the detector and the other using the TA0003 distribution. These two simulation sets were produced using the same events were processed through the IceCube Monte Carlo simulation and pass through the same IceCube processing chain to the final analysis level of an update to the IC86.2011 sterile neutrino analysis [26]. Here, the events that pass the cuts at the final analysis level are >99.9% upward-going (a trajectory oriented upwards relative to the horizon) secondary muons produced by charged current muon neutrino/antineutrino interactions. The event selection criteria is described in Ref. [27]. The muon reconstructed energy range of this event selection is between approximately 500 GeV and 10 TeV.

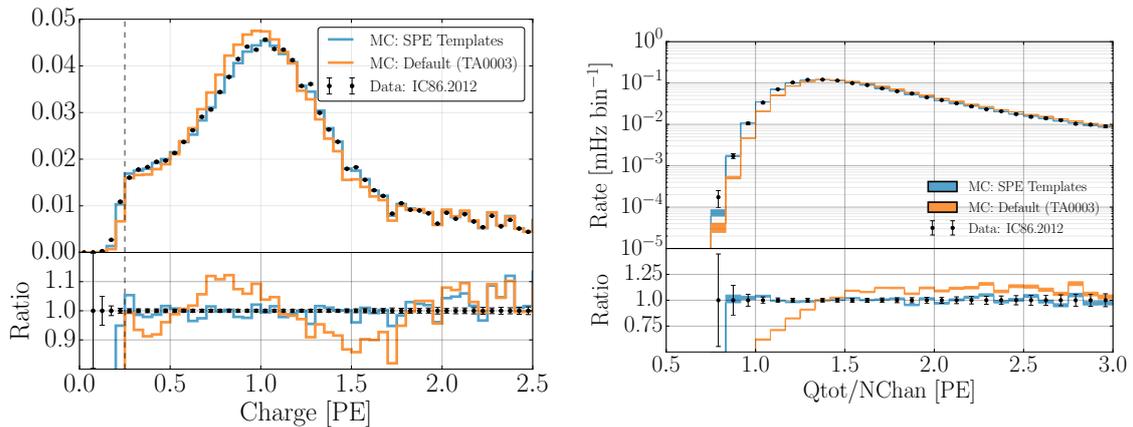


Figure 11. A comparison between IC86.2012 (black data points with statistical-only uncertainties) to two sets of simulation at an IceCube analysis level. Both simulation sets were produced with identical procedures, except for one describing the SPE charge distribution using the SPE charge templates (blue) and the other using the original TA0003 (orange) model for describing the SPE charge distribution in Monte Carlo. The simulation is compared to the 2012 IceCube season. The data is shown in black. Left: The total measured charge per DOM, per neutrino event at analysis level. Right: The distribution of the total measured charge of an event (Q_{tot}) per DOM, divided by the number of DOMs (N_{Chan}) that participated in the event.

Fig. 11 (left) shows the distribution a histogram of the total measured charge during each event per DOM (data points) per DOM, during each neutrino interaction, after noise removal. The black data points represent the measured IC86.2012 data but are statistically equivalent to the other seasons. The simulation set using the TA0003 charge distribution is shown in orange, and that using the SPE charge

templates is shown in blue. ~~The data is shown for the full IC86.2012 season but is statistically equivalent to any of the other seasons.~~ Fig. 11 (right) shows the distribution of the total measured charge of an event divided by the number of channels (NChan), or DOMs, that participated in the event. Both plots in Fig. 11 have been normalized such that the area under the histograms is the same.

The SPE charge templates clearly improve the overall MC description of these two variables. This update may be useful for analyses that rely on low-occupancy events (low-energy or dim events) in which average charge per channels is below 1.5 PE, and will be investigated further within IceCube.

5 Conclusion

This article outlines the procedure used to extract the SPE charge templates for all in-ice DOMs in the IceCube detector using in-situ data from IC86.2011 to IC86.2016. The SPE charge templates represent an update to the modeled single photoelectron charge distribution previously used by IceCube, the TA0003 distribution. The result of this measurement was shown to be useful for improving the overall data/MC agreement for an IceCube analysis as well as calibration of the individual PMTs. It also prompted a comparison between the shape of the SPE charge templates for a variety of hardware configurations and time dependent correlations.

The subset of HQE DOMs were found to have a smaller peak-to-valley ratio relative to the Standard QE DOMs, as well as an overall $3.17 \pm 0.01\%$ lower average charge. It was also found that the DOMs instrumented with the old toroids used for AC coupling (the first PMTs to be manufactured by Hamamatsu) had narrower Gaussian component ~~corresponding resulting in an average~~ and an increased peak-to-valley ratio of $14.36 \pm 0.01\%$. ~~This was found~~ By assuming a relationship between the production time and serial number, this difference was shown to be likely due to a change in the manufacturing over time rather than the actual AC coupling method. No significant time dependence in any of the fitted parameters associated with the SPE charge templates over the investigated seasons was observed. A reassessment of the PMT

gain settings found a systematic bias of $1.47 \pm 0.04\%$ with a standard deviation of 2.62%.

The SPE charge templates were inserted into the MC simulation and the results were compared to the default TA0003 distribution. A significant improvement in the description of the variables total charge per DOM and total charge over the number of channels was shown. Analyses which rely on low-light occupancy measurements, ~~may~~will benefit from this update. As shown in the bright-to-dim ratios, the ~~average~~ average charge for various light levels will not be affected by this update.

Acknowledgments

We acknowledge the support from the following agencies:

USA – U.S. National Science Foundation-Office of Polar Programs, U.S. National Science Foundation-Physics Division, Wisconsin Alumni Research Foundation, Center for High Throughput Computing (CHTC) at the University of Wisconsin-Madison, Open Science Grid (OSG), Extreme Science and Engineering Discovery Environment (XSEDE), U.S. Department of Energy-National Energy Research Scientific Computing Center, Particle astrophysics research computing center at the University of Maryland, Institute for Cyber-Enabled Research at Michigan State University, and Astroparticle physics computational facility at Marquette University; Belgium – Funds for Scientific Research (FRS-FNRS and FWO), FWO Odysseus and Big Science programmes, and Belgian Federal Science Policy Office (Belspo); Germany – Bundesministerium für Bildung und Forschung (BMBF), Deutsche Forschungsgemeinschaft (DFG), Helmholtz Alliance for Astroparticle Physics (HAP), Initiative and Networking Fund of the Helmholtz Association, Deutsches Elektronen Synchrotron (DESY), and High Performance Computing cluster of the RWTH Aachen; Sweden – Swedish Research Council, Swedish Polar Research Secretariat, Swedish National Infrastructure for Computing (SNIC), and Knut and Alice Wallenberg Foundation; Australia – Australian Research Council; Canada – Natural Sciences and Engineering Research Council of Canada, Calcul Québec, Compute Ontario, Canada Foundation for Innovation, WestGrid, and Compute Canada; Denmark – Villum Fonden, Danish National Research Foundation (DNRF), Carlsberg Foundation; New Zealand – Marsden Fund; Japan – Japan Society for Promotion of Science (JSPS) and Institute for Global Prominent Research (IGPR) of Chiba University; Korea – National Research Foundation of Korea (NRF); Switzerland – Swiss National Science Foundation (SNSF); United Kingdom – Department of Physics, University of Oxford.

References

- [1] F. Halzen and S. R. Klein, *Invited review article: Icecube: an instrument for neutrino astronomy*, *Review of Scientific Instruments* **81** (2010) 081101.
- [2] J. Ahrens et al., *IceCube preliminary design document*, URL: <https://icecube.wisc.edu/icecube/static/reports/IceCubeDesignDoc.pdf> (2001) .
- [3] A. Achterberg et al., *First year performance of the IceCube neutrino telescope*, *Astroparticle Physics* **26** (2006) 155–173, [[arXiv:astro-ph/0604450v2](https://arxiv.org/abs/astro-ph/0604450v2)].
- [4] M. G. Aartsen et al., *Evidence for high-energy extraterrestrial neutrinos at the IceCube detector*, *Science* **342** (2013) 1242856, [[arXiv:1311.5238v2](https://arxiv.org/abs/1311.5238v2)].
- [5] R. Abbasi et al., *The design and performance of IceCube DeepCore*, *Astroparticle Physics* **35** (2012) 615–624, [[arXiv:1109.6096v1](https://arxiv.org/abs/1109.6096v1)].
- [6] R. Abbasi et al., *The IceCube data acquisition system: Signal capture, digitization, and timestamping*, *NIM-A* **601** (2009) 294–316, [[arXiv:0810.4930v2](https://arxiv.org/abs/0810.4930v2)].
- [7] M. Aartsen et al., *Measurement of South Pole ice transparency with the IceCube LED calibration system*, *NIM-A* **711** (2013) 73–89, [[arXiv:1301.5361v1](https://arxiv.org/abs/1301.5361v1)].
- [8] R. Abbasi et al., *IceTop: The surface component of IceCube*, *NIM-A* **700** (2013) 188–220.
- [9] R. Abbasi et al., *Calibration and characterization of the IceCube photomultiplier tube*, *NIM-A* **618** (2010) 139–152, [[arXiv:1002.2442v1](https://arxiv.org/abs/1002.2442v1)].
- [10] M. G. Aartsen et al., *The IceCube Neutrino Observatory: Instrumentation and Online Systems*, *JINST* **12** (2017) 1748–0221, [[arXiv:1612.05093v2](https://arxiv.org/abs/1612.05093v2)].
- [11] M. Aartsen et al., *Energy reconstruction methods in the IceCube Neutrino Telescope*, *JINST* **9** (2014) 1748–0221, [[arXiv:1311.4767v3](https://arxiv.org/abs/1311.4767v3)].
- [12] R. Stokstad, *Design and performance of the IceCube electronics*, URL: <https://cds.cern.ch/record/920022/files/p20.pdf> (2005) .
- [13] Hamamatsu, *Resources: Basics and Applications*, URL: https://www.hamamatsu.com/resources/pdf/etd/PMT_handbook_v3aE.pdf (2018) .
- [14] Hamamatsu, *Handbook Resources, Chapter 4*, URL: https://www.hamamatsu.com/resources/pdf/etd/PMT_handbook_v3aE-Chapter4.pdf (2018) .

- [15] J. Brack et al., *Characterization of the Hamamatsu R11780 12 in. photomultiplier tube*, *NIM-A* **712** (2013) 162–173, [[arXiv:1210.2765v2](#)].
- [16] E. Calvo et al., *Characterization of large-area photomultipliers under low magnetic fields: Design and performance of the magnetic shielding for the Double Chooz neutrino experiment*, *NIM-A* **621** (2010) 222–230, [[arXiv:0905.3246v1](#)].
- [17] F. Kaether and C. Langbrandtner, *Transit time and charge correlations of single photoelectron events in R7081 photomultiplier tubes*, *JINST* **7** (2012) P09002, [[arXiv:1207.0378v2](#)].
- [18] B. Lubsandorzhev, P. Pokhil, R. Vasiljev and A. Wright, *Studies of prepulses and late pulses in the 8" electron tubes series of photomultipliers*, *NIM-A* **442** (2000) 452–458.
- [19] K. Ma et al., *Time and amplitude of afterpulse measured with a large size photomultiplier tube*, *NIM-A* **629** (2011) 93–100, [[arXiv:0911.5336v1](#)].
- [20] S. Torre, T. Antonioli and P. Benetti, *Study of afterpulse effects in photomultipliers*, *Review of Scientific Instruments* **54** (1983) 1777–1780.
- [21] Hamamatsu, *Photomultiplier tubes: Construction and Operating Characteristics*, URL: https://www.hamamatsu.com/resources/pdf/etd/PMT_TPMZ0002E.pdf (2016) .
- [22] M. Aartsen et al., *Characterization of the atmospheric muon flux in IceCube*, *Astroparticle Physics* **78** (2016) 1–27, [[arXiv:1506.07981v2](#)].
- [23] W. R. Leo, *Techniques for nuclear and particle physics experiments: a how-to approach*. Springer Science & Business Media, 2012.
- [24] M. Aartsen et al., *Search for steady point-like sources in the astrophysical muon neutrino flux with 8 years of IceCube data*, *The European Physical Journal C* **79** (2019) 234, [[arXiv:1811.07979v2](#)].
- [25] R. Dossi, A. Ianni, G. Ranucci and O. J. Smirnov, *Methods for precise photoelectron counting with photomultipliers*, *NIM-A* **451** (2000) 623–637.
- [26] M. Aartsen et al., *Searches for sterile neutrinos with the IceCube detector*, *Physical Review Letters* **117** (2016) 071801, [[arXiv:1605.01990v2](#)].
- [27] M. Aartsen, K. Abraham, M. Ackermann, J. Adams, J. Aguilar, M. Ahlers et al.,

Evidence for astrophysical muon neutrinos from the northern sky with icecube, Physical review letters **115** (2015) 081102.